



ASTRO-H

INSTRUMENT CALIBRATION REPORT SXS DETECTOR GAIN ASTH-SXS-CALDB-GAINPIX

Version 0.1

12 March 2016

ISAS/ GSFC

Prepared by: Megan Eckart, Maurice Leutenegger, F. Scott Porter, Caroline Kilbourne, and the SXS Instrument Team

Table of Contents

Introduction.....	4
1.1 Purpose.....	4
1.2 Scientific Impact.....	4
2 Release CALDB 20160310.....	5
2.1 Data Description.....	5
2.2 Data Analysis.....	8
2.3 Results.....	10
2.4 Final Remarks.....	11
3 References.....	11

CHANGE RECORD PAGE (1 of 1)

DOCUMENT TITLE: SXS Detector Gain			
ISSUE	DATE	PAGES AFFECTED	DESCRIPTION
Version 0.1	March 2016	All	First Release

Introduction

1.1 Purpose

This document describes the parameterization of the SXS energy gain scale – the relationship between the measured signal and the incident photon energy. Each pixel requires its own gain correction, and the gain must be specified independently for each grade. We derive a non-linear function that describes the gain scale and parameters that describe how the function changes with instrument operating conditions.

The specific nature of any change in operating condition will determine whether the corresponding gain change is linear (a stretch of the gain curve) or non-linear (a change in shape of the gain curve). The gain of each SXS pixel depends linearly on the (small) gain–temperature coefficient of the room temperature amplifiers and has a non-linear scaling with detector temperature. The detector temperature depends on the CTS temperature setpoint as well as loading on the control thermometers and detector pixels due to nearby structures such as the detector assembly structure (~1.2–1.6K) and the inner vapor cooled shield (IVCS; ~22–35K). These effects tend to change the detector temperatures of all array pixels together. There is also differential radiative loading related to the screening of long wavelength radiation that varies depending on pixel position in the array (i.e., inner pixels are better screened than outer pixels).

We measured the detector gain for each pixel for several detector temperature setpoints in the otherwise nominal ground operating conditions (He mode). These measurements are detailed in Section 2, and the resulting gain parameters are included in the CALDB. From this initial set of gain curves and the measurement of a fiducial line as a function of time during each observation –either using the calibration pixel or pixel-by-pixel– the software pipeline generates an appropriate gain curve that may be used to convert PHA to EPI.

1.2 Scientific Impact

The SXS gain coefficients are used to assign energies for each event via the combination of tasks `sxsgain` and `sxspha2pi`. The hires coefficients are used in `sxsgain` to calculate a time-dependent effective gain temperature that is used as an input to `sxspha2pi`. The gain coefficients are used in `sxspha2pi` to construct energy verses PHA curves for each effective temperature and each event grade; the resulting curves are applied to convert PHA to EPI. This gain table is sufficient to provide an accurate energy for primary events of all grades (hires, midres primaries, and lores primaries).

2 Release CALDB 20160310

Filename	Valid data	Release data	CALDB Vrs	Comments
ah_sxs_gainpix_20140101v001.fits	2014-01-01	20160310	001	Original ASCII files: gain_49mK_SXS_v2.0.txt gain_50mK_SXS_v2.0.txt gain_51mK_SXS_v2.0.txt SHPTEMPL=2015-03-10

2.1 Data Description

The calibration measurements of the SXS detector gain were performed in March 2015 during SXS instrument-level testing at Tsukuba Space Center (TKSC) using the flight version of the electronics boxes (XBOX, ADRC). The SXS dewar was in its final flight configuration, following the installation of the isolators between the dewar and the cryocoolers.

We used a Rotating Target X-ray Source (RTS) positioned above the dewar to provide x-ray lines at known energies from 4.5–13.5 keV. Figure 1 presents a photo of the experimental setup. Calibration at low x-ray energies was not possible at TKSC due to the presence of the gate valve's beryllium window.

The RTS consists of a bright x-ray continuum source (TruFocus model 5110 with tungsten target) that illuminates targets mounted on a rotating wheel. Fluorescence from the targets provides x-ray line emission directed to the instrument aperture. The targets are typically single crystal and are adjusted to steer Bragg-reflected photons away from the detector. For the case of the gain measurements we used the following targets in the eight slots: 0) Fe, 1) KBr, 2) Cu, 3) GaAs, 4) Co, 5) Cr, 6) Mn, 7) TiO₂. The x-ray source settings were HV = 20kV and $I_{\text{emission}} = 30\mu\text{A}$ (for 49mK and 50mK hires data) or = $40\mu\text{A}$ (for 50mK midres and 51mK hires data) and the dwell time at each target was one minute, providing approximately 1 ct/s/pixel.

The data were acquired using the Pulse Shape Processor (PSP). The PSP calculates the PHA of each event onboard. For hires and midres grades the events are optimally filtered and the result is assigned to the PHA column of the event file. Please see Szymkowiak et al. (1993) and Boyce et al. (1999) for background on optimal filtering for microcalorimeters. Hires events are calculated using a 1024-sample optimal filter while midres events are calculated using a 256-sample optimal filter. Each pixel has a hires and midres optimal filter template stored onboard, and a given set of the 72 filter templates are identified by the SHPTEMPL keyword. The current optimal filter templates were calculated during the calibration phase in March 2015 and assigned SHPTEMPL = 2015-03-10.

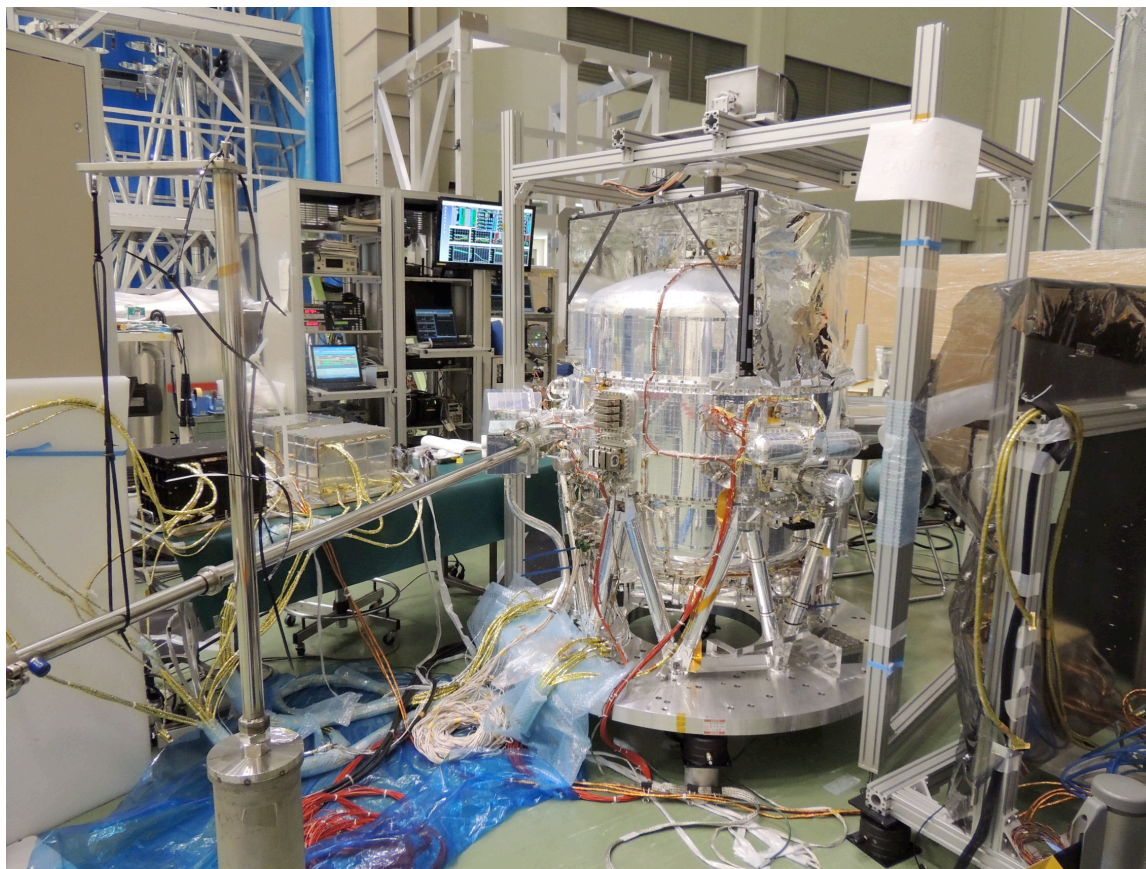


Figure 1 Rotating Target X-ray Source (RTS) mounted above the flight instrument in March 2015.

Lores events are not optimally filtered in the PSP; instead their pulse height is given by maximum ADC value in the sample record (after subtracting the baseline value of the sample). In fact, this ‘lores pulse height’ is calculated not just for lores events but for events of all grades. For hires and midres events the result is placed in the LO_RES_PH column whereas for lores events it fills both the LO_RES_PH and the PHA columns. Because the LO_RES_PHA is telemetered for all event grades, we acquire simultaneous lores gain scale information during experiments aimed at calibrating hires or midres event grades.

To acquire spectra for the hires and lores gain scales we operate the PSP in its normal mode. For the hires gain scale we derive curves by relating the PHA (ADC units) to energy (eV) using hires events. For the lores gain scale we use all primary events (hires, midres primaries, and lores primaries) but relate the LO_RES_PHA (ADC units) to energy (eV).

To obtain a sufficient number of midres events in a reasonable exposure time, both in the case of our relatively low count-rate energy scale calibration setup at TKSC and for appropriate celestial sources, we operate the PSP in forced midres mode. In this mode hires-graded events are processed as if they were midres (using the 256-sample optimal filter template) so that both hires and midres events may be combined to measure a midres gain scale by relating the PHA (ADC units) to energy (eV).

Based on analyses of gain curves measured over a wide span of instrument operating conditions, including in cryogen free mode, we find that we may treat all gain variations as equivalent to changes in detector temperature. As a result, we use the following approach. For each event grade we provide gain curves at three bath temperatures. The intention is that the resulting gain curves will envelope the gain curves we are apt to encounter during the mission lifetime. These curves are then used in the software pipeline, in conjunction with a measured fiducial line, to construct a gain curve appropriate for the instantaneous operating conditions of the instrument. See Porter et al. (2015) for details about this non-linear drift correction approach. In nominal operating conditions on the ground the instrument gain is typically very close to the 50mK gain curve and the gain correction applied by the pipeline is approximately a small linear stretch to the 50 mK gain curve.

Each gain calibration experiment was recorded as an Igor Pro experiment using the XRSGSE software suite version 10.5.1. Table 1 provides the experiment names as well as the start and stop times of each exposure, while Table 2 presents selected operating parameters for onboard SXS electronics boxes (PSP, XBOX, and ADRC) and relevant operating temperatures.

Temp [mK]	Hires/Lores experiment name	Hires/Lores Start Time [UT]	Hires/Lores Stop Time [UT]	Midres experiment name	Midres Start Time [UT]	Midres Stop Time [UT]
49.0	15-03-11.07.48.06Z	3/11/2015 08:03	3/11/2015 16:01	n/a	n/a	n/a
50.0	15-03-11.16.24.16Z	3/11/2015 16:25	3/12/2015 04:38	15-03-12.13.56.25Z	3/12/2015 13:59	3/13/2015 01:08
51.0	15-03-13.01.40.55Z	3/13/2015 01:41	3/13/2015 09:40	n/a	n/a	n/a

Table 1 Experiment files and start/stop times for the gain calibration measurements. The lores gain parameters are derived using the LOW_RES_PH of all primary events; a separate experiment is not required. For the midres experiment the PSP was in forced midres mode.

PSP Parameters		Comments
Thresholds	pix 10,15-17,21-22,25,28-31,34 = 24; pix 0-7,11-12,14,19,24,32-33,35 = 25; pix 13,18,23 = 26; pix 9 = 28; pix 8 = 32; pix 20 = 29; pix 27 = 40; pix 26 = 62	PULSE_THRES and NOISE_THRES are set to these values. A threshold of 25 corresponds to ~34 eV.
Templates	SHPTEMPL=2015-03-10	
Average pulse scale	pix 0-35 = 144000	PSP parameter PHA_AVGPULSE
Software Version	0x150310	
XBOX Parameters		
Detector Bias Setpoint	1.60784V	0x0052 in hex
Detector Bias Readback	1a=1.582V, 1b=1.585V, 2a=1.583V, 2b=1.588V	
ADRC Parameters and Relevant Temperatures		
CTS Temperature Setpoint	49.0 / 50.0 / 51.0 mK	See column 1 of Error! Reference source not found.
Control Thermometer	CT0 Sensor0	
DA Temperature	1.220–1.232 K	He mode operation
He Tank Temperature	1.216–1.227 K	
IVCS Temperature	26.5–26.9 K	

Table 2 Selected instrument parameters during SXS gain calibration.

2.2 Data Analysis

Overview

For each experiment we follow a standard procedure to determine the detector gain curve. The following prescription is performed independently for each of the array pixels. First, we apply a linear drift correction to the data, if necessary, to remove very small changes in effective detector temperature over the course of the exposure. Next, we histogram the events with bin width of ~1 ADC unit (~0.5 eV). We then fit each of the x-ray line complexes to determine a set of PHA–energy pairs and associated error estimates. Finally, we fit these data to the fourth-order polynomial given in Eq (1):

$$E \text{ [eV]} = c1*PHA + c2*PHA^2 + c3*PHA^3 + c4*PHA^4. \quad \text{Eq. (1)}$$

One exception is the calibration pixel (pixel 12). Since it only receives photons from the collimated ^{55}Fe source, not from the instrument aperture, we must derive its gain scale from fits to two only line complexes (Mn $K\alpha$ and $K\beta$). Therefore, we constrain the fit function to a second order polynomial ($c3=c4=0$).

To allow for greater flexibility in the CALDB, in addition to terms c1–c4, we also include the option of a linear offset term (c0) and a fifth order term (c5); however, the current gain files have each of these terms set to zero for all pixels.

Hires

For each of the three heatsink temperatures we make spectra for each pixel using hires events. We fit the following line complexes: Ti K α , Cr K α , Mn K α , Fe K α , Co K α , Cu K α , Ga K α , As K α , and Br K α .

Midres

We acquired data at 50 mK in forced midres mode, in which both hires and midres events are processed with the 256-sample (midres) optimal filter template (as described in Section 2.1), allowing much more efficient data collection for midres-processed pulses. We use the same set of x-ray line complexes as described for the hires gain.

A linear stretch (~ 0.9998) has been applied to the resulting 50 mK midres gain scales to correct for a slight difference in the effective temperature during the forced midres exposure as compared to the 50 mK hires exposure.

We did not have time to acquire data in forced midres mode at 49mK and 51mK prior to delivery to the spacecraft. Instead, we calculate the gain components by scaling the 50 mK midres gain curve by the ratio of the 49 mK (or 51 mK) hires gain curve to the 50 mK hires gain curve, and then fitting a 4th order polynomial to the resulting curve. We tested the efficacy of this approach by evaluating the (low-statistics) midres primary lines obtained during the 49/51 mK hires experiments and found that the results give errors of less than 5 eV at 49mK and less than 10 eV at 51 mK. These are deemed acceptable for nominal cryogen mode observations since we operate very close to the 50 mK gain curves given in the CALDB.

Lores

We used the LO_RES_PHA of primary events of all grades, as described in Section 2.1, and fit the same set of lines to determine the gain curves at each temperature. Since the lores data were acquired simultaneously with the hires data, the reference effective temperature for each dataset was by definition the same and did not require additional processing (as in the case of the midres data).

2.3 Results

The resulting gain parameters for each pixel and each event grade are given in the CALDB file. The following plots give examples of the gain curves, for reference. The residuals on the fits are within ± 0.5 eV for the hires and midres gain curves and ± 2.5 eV for the lores gain curves over the range 4.5–12 keV.

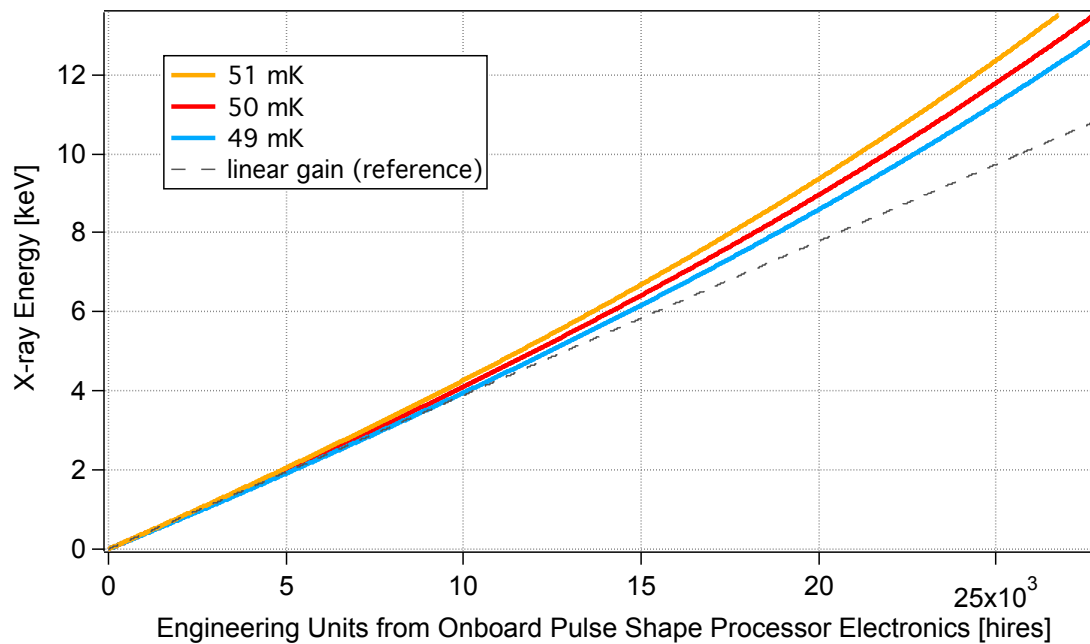


Figure 2 Hires gain scales for pixel 0 calculated using the polynomial coefficients given in the CALDB file. The 49 mK and 51 mK gain scales bound the gain conditions we expect to encounter on-orbit.

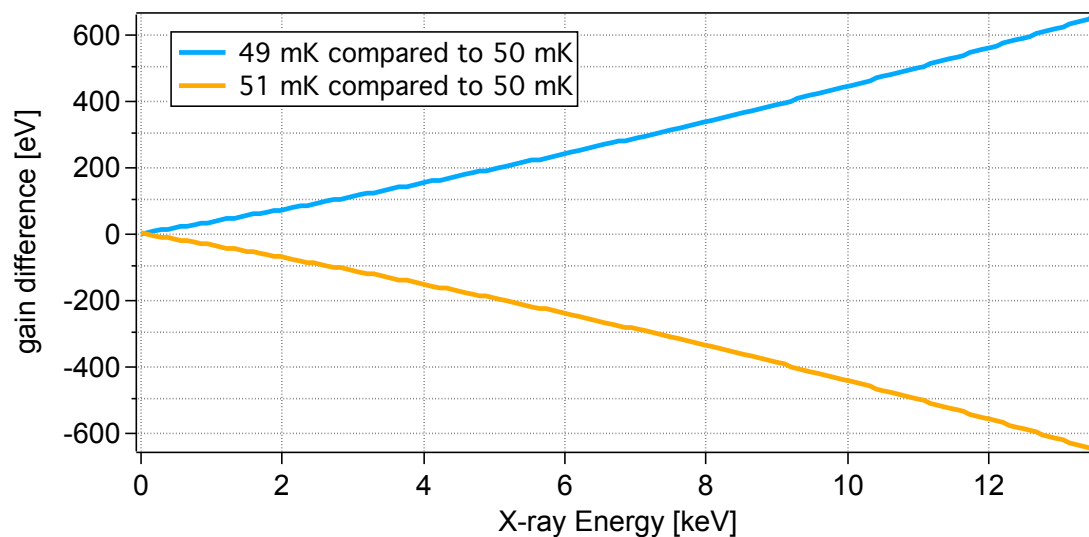


Figure 3 This plot highlights the difference in gain between the hires gain scales at different heatsink temperatures.

2.4 Final Remarks

During initial in-flight calibration we plan to check the SXS gain using a combination of on-board sources and celestial sources for a set of operating conditions (49mK, 50mK, 51mK; and in forced midres mode at each temperature). Our aim is to have parameterized the gain in such a way that even if operating conditions change slightly, the change in gain is wholly described by a change in effective temperature, and will not require new CALDB files. However, we expect that the addition of low-energy lines in the calibration measurements as well as the forced midres data at 49 and 51 mK will produce changes significant enough to warrant a new release.

If at any time the optimal filter templates (keyword SHPTMPL) for one or more pixel are changed on-orbit then the gain calibration for hires and midres event grades will need to be modified accordingly. While we intend to use these same optimal filter templates for the entirety of the mission so as not to invalidate the ground calibration, if the on-orbit noise conditions change substantially then we will consider changing the optimal filter templates.

In addition to the data used to create the current CALDB gain curves, we also acquired ground calibration data at TKSC over an extended energy bandpass – to energies of 25 keV. These data are not included in the current release of the CALDB, but may be incorporated at a later stage if deemed necessary. We also performed similar measurements in cryogen free mode with several combinations of CTS control temperature, detector assembly structure control temperature, and IVCS temperature. These measurements are not required for the CALDB, but were essential in verifying our approach and confirming that the 49mK/51mK He-mode data envelope the gain conditions we expect during cryogen free mode.

And finally, we re-emphasize that these gain curves will only provide precise energies for primary events. An additional correction is required to recover the energy of secondaries. While an initial CALDB file exists to aid in correcting midres secondaries (CALDB filename = `ah_sxs_secpulse_20140101v001.fits`), the requisite algorithm is not yet implemented in the software.

3 References

- [1] K.R. Boyce, M.D. Audley, R.G. Baker, J.J. Dumonthier, R. Fujimoto, K.C. Gendreau, Y. Ishisaki, R.L. Kelley, C.K. Stahle, A.E. Szymkowiak, and G.E. Winkert. “Design and performance of the ASTRO-E/XRS signal processing system,” *Proc. SPIE*, **3765**, 741-750 (1999).
- [2] F.S. Porter, M.P. Chiao, M.E. Eckart, R. Fujimoto, Y. Ishisaki, R.L. Kelley, C.A. Kilbourne, M.A. Leutenegger, D. McCammon, K. Mitsuda, M. Sawada, A.E. Szymkowiak, Y. Takei, M. Tashiro, M. Tsujimoto, T. Watanabe, and S. Yamada. “Temporal Gain Corrections for X-ray Calorimeter Spectrometers,” *Journal of Low Temperature Physics*, p1-7 (2016). DOI: 10.1007/s10909-016-1503-2.
- [3] A.E. Szymkowiak, R.L. Kelley, S.H. Moseley, and C.K. Stahle. “Signal processing for microcalorimeters,” *JLTP*, **93**, 281-285 (1993).